



# The Teleflex Medical OEM Hydrophilic Coating Performs Favorably for Lubricity and Durability\*

## Teleflex Medical OEM Coating vs Competitors

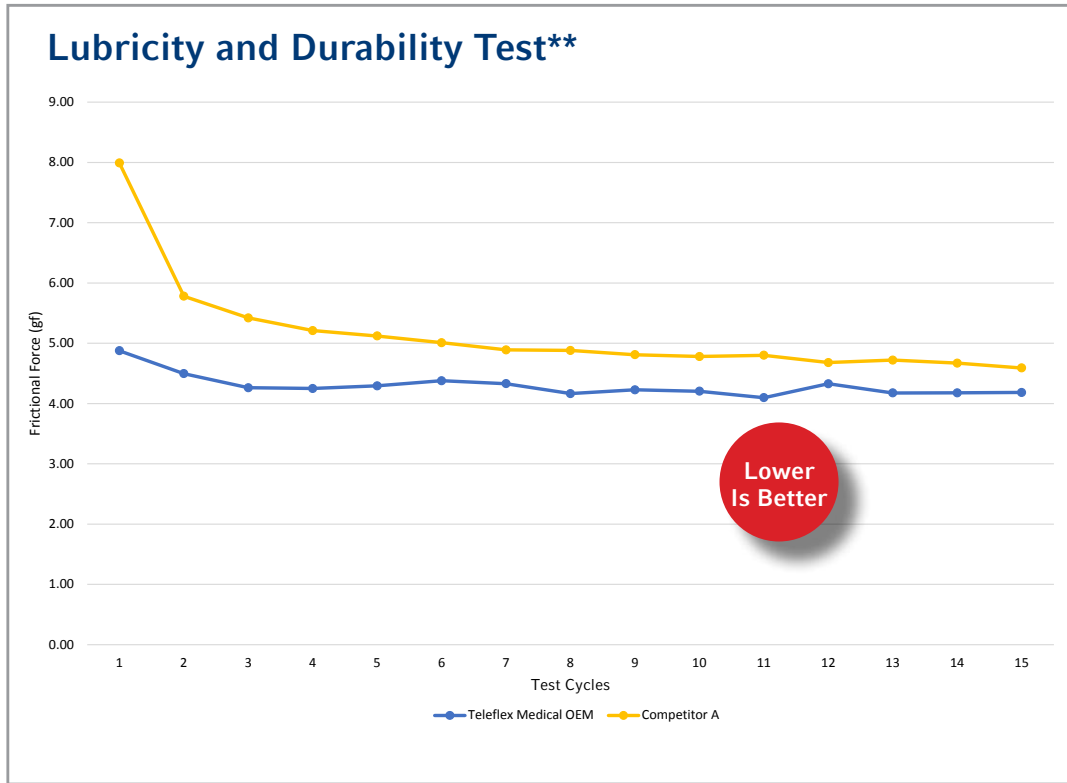

\*Please note:  
 • Testing data in master file

\*\*Please note:  
 • Tested in-house using a Harland FTS Friction Test System  
 • Tested on Pebax®-based substrates

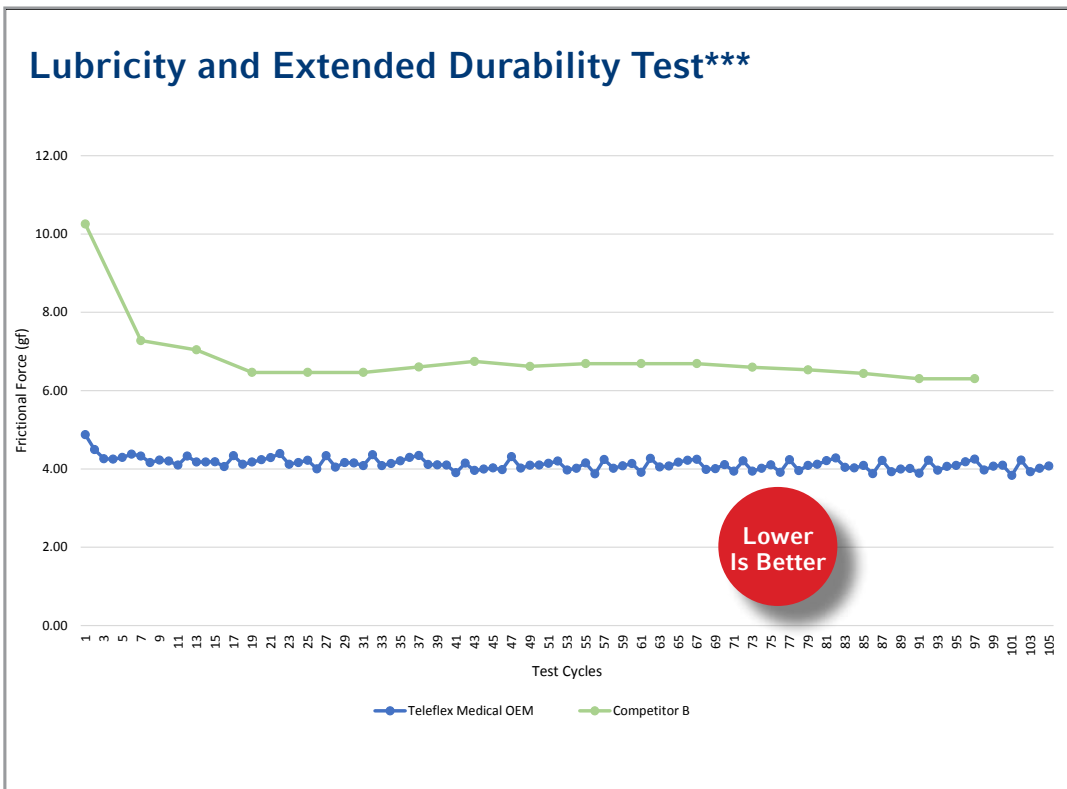

\*\*\*Please note:  
 • Competitor data from its website. This graph displays the resistance force needed to pull a coated sample between silicone rubber pads clamped on the sample with 500 grams clamping force.  
 • Comparable testing of Teleflex Medical OEM coating using a Harland Friction Test System  
 • Tested on Pebax®-based substrates



Work With The Experts™  
[www.teleflexmedicoem.com](http://www.teleflexmedicoem.com)